Recommended File Sequence TriAuto ZX2 with EndoWave for Standard Straight and Curved Canals

Step 1
Upper Part Shaping
(Coronal Flaring)

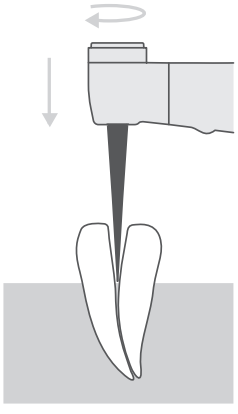

Step 2 / OGP
Glide Path

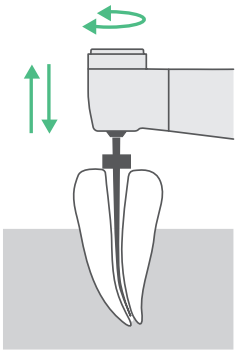

Step 3 / OTR
OTR Canal Shaping

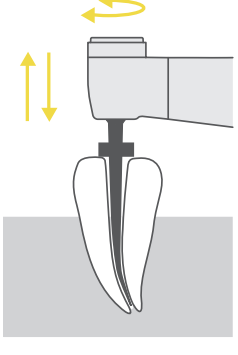

Description	Recommended sequence	
	Recommended files	Recommended memory
Canal Measurement (Apex Location) Separate measurement only necessary for documentation reasons	● k-file handfile #10	m1
Step 1 **Upper Part Shaping (Coronal Flaring)** Enlarge the upper part of the canal to make treatment easier	◆● EndoWave NiTi-Files 08/#35/19mm Order no. 6820-835	m2
Step 2 **Glide Path** Use a thin file to create the glide path If the contrary electrode is applied to the patient, the instrument is linked to the canal measurement function while it is being used.	◆● EndoWave NiTi-Files 02/#10/25mm Order no. 6825-210	m3
	◆● EndoWave NiTi-Files 02/#15/25mm Order no. 6825-215	m3
	◆● EndoWave NiTi-Files 02/#20/25mm Order no. 6825-220	m3
Step 3 **OTR Canal Shaping** Change the file size as you shape the canal If the contrary electrode is applied to the patient, the instrument is linked to the canal measurement function while it is being used.	◆● EndoWave NiTi-Files 04/#15/25mm Order no. 6825-415	m4
	◆● EndoWave NiTi-Files 04/#25/25mm Order no. 6825-425	m4
	◆● EndoWave NiTi-Files 04/#30/25mm Order no. 6825-430	m4
	◆● EndoWave NiTi-Files 04/#35/25mm Order no. 6825-435	m4
	◆● EndoWave NiTi-Files 06/#35/25mm Order no. 6825-635	m4

◆ Included in the starter kit
◆ Order these files seperate if needed
● Recommended sequence
● Use these sequence if necessary

Recommended File Sequence TriAuto ZX2 with EndoWave for Advanced Complex and High Difficulty Canals

Step 1
Upper Part Shaping
(Coronal Flaring)

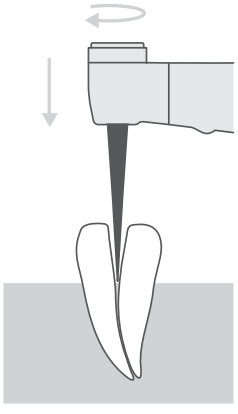

Step 2 / OGP
Glide Path

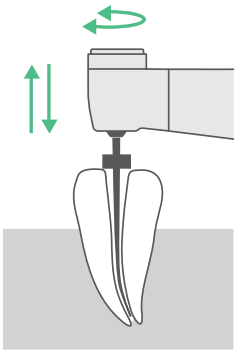

Step 3 / OTR
OTR Canal Shaping

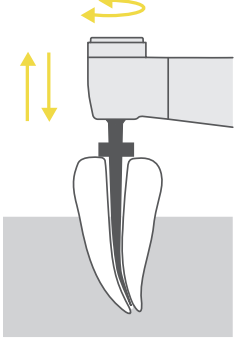

Description	Recommended sequence	
	Recommended files	Recommended memory
Canal Measurement (Apex Location) Separate measurement only necessary for documentation reasons	● k-file handfile #10	m1
Step 1 **Upper Part Shaping (Coronal Flaring)** Enlarge the upper part of the canal to make treatment easier	◆● EndoWave NiTi-Files 08/#35/19mm Order no. 6820-835	m2
Step 2 **Glide Path** Use a thin file to create the glide path If the contrary electrode is applied to the patient, the instrument is linked to the canal measurement function while it is being used.	◆● EndoWave NiTi-Files 02/#10/25mm Order no. 6825-210	m3 / m5
	◆● EndoWave NiTi-Files 02/#15/25mm Order no. 6825-215	m3 / m6
	◆● EndoWave NiTi-Files 02/#20/25mm Order no. 6825-220	m6
Step 3 **OTR Canal Shaping** Change the file size as you shape the canal If the contrary electrode is applied to the patient, the instrument is linked to the canal measurement function while it is being used.	◆● EndoWave NiTi-Files 04/#15/25mm Order no. 6825-415	m6
	◆● EndoWave NiTi-Files 04/#25/25mm Order no. 6825-425	m7
	◆● EndoWave NiTi-Files 04/#30/25mm Order no. 6825-430	m7
	◆● EndoWave NiTi-Files 04/#35/25mm Order no. 6825-435	m7
	◆● EndoWave NiTi-Files 06/#35/25mm Order no. 6825-635	m7

◆ Included in the starter kit
◆ Order these files seperate if needed
● Recommended sequence
● Use these sequence if necessary

Subject to technical changes and errors.
JME EN FA 0517*1.